




WELL D-ONE® SYSTEM

UROGEN WELL D-ONE®

System for the presumptive identification and AST of:
Mycoplasma hominis, *Mycoplasma spp.*, *Ureaplasma urealyticum/parvum*
Neisseria spp., *Streptococcus B*, *Staphylococcus aureus*,
Enterococcus spp., *Escherichia coli*, *Gardnerella vaginalis*,
Trichomonas vaginalis and *Candida spp.*

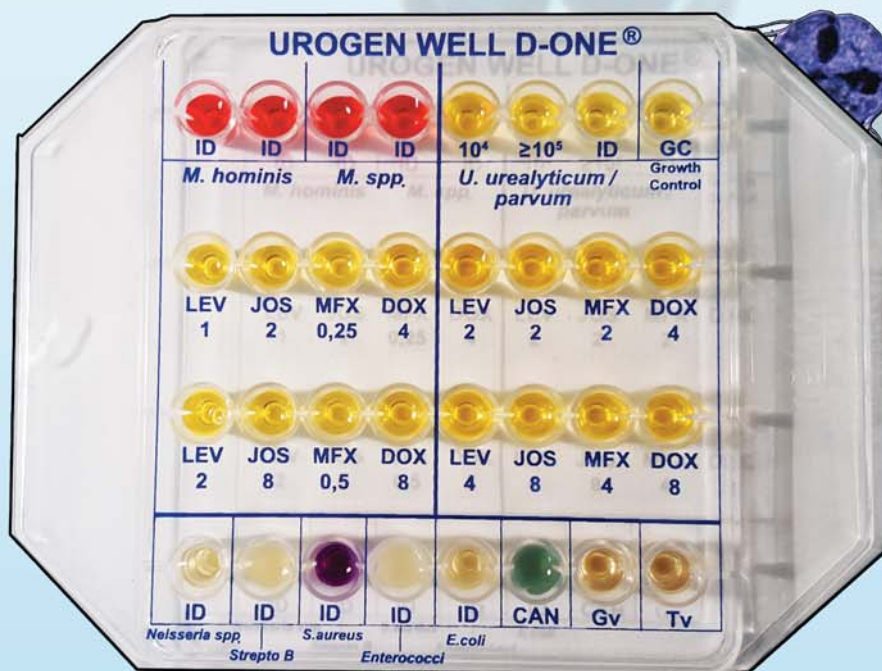

The tested sample is diluted in accordance with the procedure and inoculated directly into the wells of the plate. Incubation is performed for 18-24-48 hours and readings are taken visually without additional equipment.

The results are evidenced by color changes that occur inside the wells according to reactions caused by chemical or chromogenic components contained in specific formulations for each microorganism.